



9 Position Dura-Mag™ Magnetic Stirrer

CLS-4100-09



OPERATIONS MANUAL

3800 North Mill Road • Vineland, NJ 08360 • USA
Tel: 1-800-843-1794 • Fax: 1-800-922-4361
Web: www.cglifesciences.com

REV: F

FEATURES

1. Trouble free brushless motor
2. Integrated power supply for 100 to 240VAC service.
3. Heavy duty magnets and drive system.
4. Stainless steel top with easy alignment marks.
5. Non-slip trouble free toothed belt design for long life.
6. Speed range from 25 to 400 rpm's.
7. Illuminated LCD display.
8. Optional output for remote communication available.
9. Optional motion alarm available

GENERAL USE

The Chemglass Life Science's nine position magnetic stirrer is a rugged design for 24/7 laboratory or production applications. It is ideal for CO2 incubators with a maximum capacity of nine 500ml spinner vessels.

SPECIFICATIONS

Supply Voltage - 120VAC to 240VAC +/-10%, 50-60 Hz

Dimensions H x W x D - (inches 3½ x 16¾ x 19¼), (centimeters - 8.9 x 42.5 x 48.9)

Ambient Temperature - 0 to 40°C, 32 to 104°F

Speed range from 25 to 400 rpm's. [+/- 1% or 1 RPM, whichever is greater]

SET-UP


(See Figure 1)

1. Connect the one end of detachable power cord to the AC/DC converter (*DC power supply*) and then connect to “INPUT 24Vdc” receptacle in rear of unit. Plug power cord into a suitable electrical outlet.
2. Place one or more spinner vessels (purchased separately) atop of unit directly over




magnet alignment marks.

9 Alignment Marks

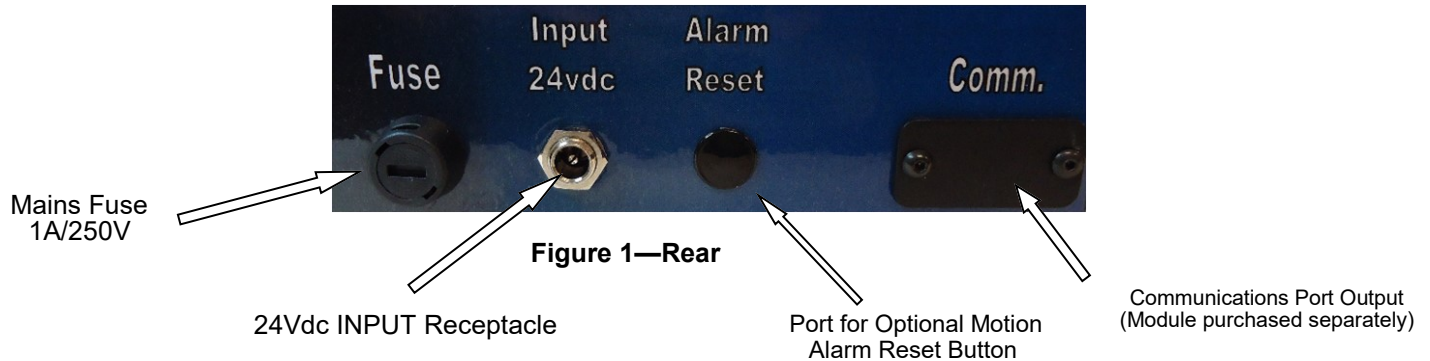

OPERATION

To operate, turn the main power switch to the “ON” position. Turn the speed control knob to set the desired rpm value. The units are designed to operate within a range of 25-400 rpm. Adjust the speed by turning the speed control knob, CW to increase speed, CCW to decrease it. The unit will ramp up (or down) to your selected speed. Turn the “LOCK” ring clockwise about an eighth of a turn to prevent any inadvertent changes to the set speed. Turn the “LOCK” ring counterclockwise to unlock the speed control knob.

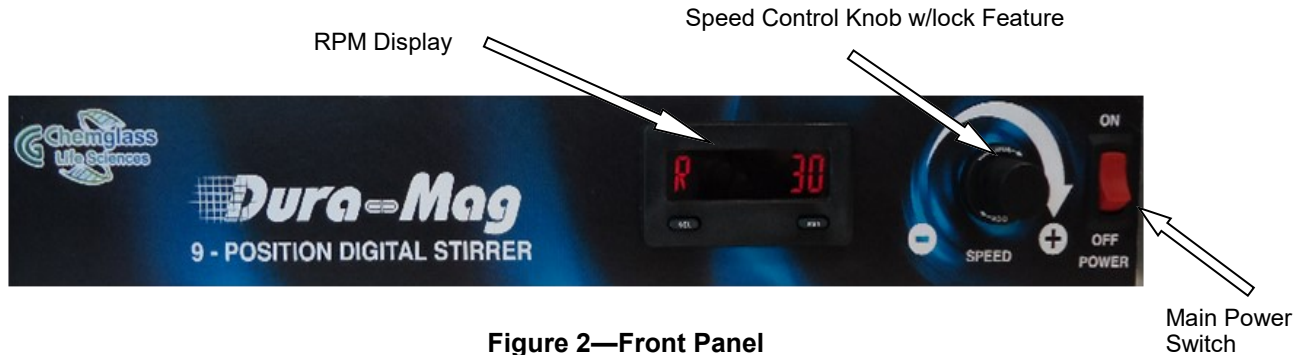

Warranty

Chemglass, Inc. guarantees this unit against defects in material and workmanship for a period of one year from the date of sale. If the unit should malfunction, it must be returned for evaluation. If the unit is determined to have a defect in materials or workmanship, then it will be repaired or replaced at no charge. Tampering with the unit or damage resulting from excessive current, heat, moisture, vibration, corrosive materials, or misuse will void this warranty. Programming changes or reconfigurations are not covered under warranty.

Return Authorization:

CGLS must authorize any return of product. Please contact a customer service representative via the correspondence listed below to obtain a Return Merchandise Authorization (RMA) number. The purchaser is responsible for all packing and shipping to CGLS. If the equipment or material came in contact or was proximate to any biological organism, toxic or corrosive material, or any agent reasonably deemed to be potentially harmful, it must be cleaned and decontaminated prior to receipt by CGLS. The purchaser is obligated to disclose fully in writing, the cleaning and decontamination method. We reserve the right not to accept any unauthorized or potentially harmful shipment.

Correspondence:

Chemglass Life Sciences
3800 North Mill Rd.
Vineland, NJ 08360
USA

Phone: 800-843-1794
Email: customer-service@cglifesciences.com
Web: www.cglifesciences.com

